


UT203+QA检测报告

检测设备: 使用仪器: FLUKE5522A

环境温度: 23.3℃/65%

功能	量程	输入	精度	范围	测试值	结果
直流电压	400mV	350.0mV	±0.7%+3	347.8~352.2mV	350.2mV	合格
	4.000V	3.500V	±0.5%+2	3.484~3.516V	3.512V	合格
	40.00V	35.00V	±0.5%+2	34.84~35.16V	34.98V	合格
	400.0V	350.0V	±0.5%+2	348.4~351.6V	350.1V	合格
交流电压	4.00V	3.500V	±1.0%+5	3.468~3.523V	3.501V	合格
	40.00V	35.00V	±0.8%+5	34.68~35.23V	34.98V	合格
	400.0V	350.0V	±0.8%+5	346.8~352.3V	349.5V	合格
交流电流	40.00A	35.00A50HZ	±2.0%+5	34.40~35.60A	35.12A	合格
	400.0A	350.0A50HZ	±2.0%+5	344.0~356.0A	351.8A	合格
直流电流	40.00A	35.00A	±2.0%+5	34.40~35.60A	35.02A	合格
	400.0A	350.0A	±2.0%+5	344.0~356.0A	350.5A	合格
电阻	400.0Ω	350.0Ω	±1.0%+2	347.0~353.0Ω	350.1Ω	合格
	4.000kΩ	3.500kΩ	±0.8%+2	3.476~3.524kΩ	3.515kΩ	合格
	40.00kΩ	35.00kΩ	±0.8%+2	34.76~35.24kΩ	35.08kΩ	合格
	400.0kΩ	350.0kΩ	±0.8%+2	347.6~352.4kΩ	350.8kΩ	合格
	4.000MΩ	3.500MΩ	±2.5%+5	3.426~3.574MΩ	3.511MΩ	合格
电容	40.00nF	35.00nF	±4.0%+5	33.84~36.16nF	35.23nF	合格
	400.0nF	350.0nF	±4.0%+5	338.4~361.6nF	352.3nF	合格
	4.000uF	3.500uF	±4.0%+5	3.384~3.616uF	3.508uF	合格
	40.00uF	35.00uF	±4.0%+5	33.84~36.16uF	35.28uF	合格
	400.0uF	350.0uF	±4.0%+5	338.4~361.6uF	351.7uF	合格
	4.000mF	3.500mF	±10%+0	3.220~3.780mF	3.537mF	合格
频率	10.00Hz	10.00Hz200mVrms	±0.1%+4	9.97~10.03Hz	10.01Hz	合格
	100.0kHz	100.0kHz200mVrms	±0.1%+4	99.3~100.7kHz	100.1kHz	合格
	10.00MHz	10.00MHz3Vpp/10MHz	±0.1%+4	9.997~10.03KHz	10.01MHz	合格
▶	4148	0.5~0.8V			0.528V	合格
⋯)	小于30欧发声				发声	合格

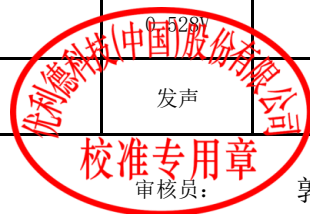

检查员: 张琼

审核员: 郭桂余