



校准证书

CALIBRATION CERTIFICATE

证书编号 GDDE202101191
Certificate No.
(代替GDDE202101135号证书)

第 1 页, 共 7 页
Page of .

委托方 优利德科技(中国)股份有限公司
Client

委托方联络信息 广东省东莞市松山湖园区工业北一路6号
Contact Information

计量器具名称 10kV高压绝缘电阻测试仪 (电子式绝缘电阻表)
Description

型号规格 UT515B
Model/Type

制造厂 UNI-T
Manufacturer

出厂编号 C213292794
Serial No.

设备编号 /
Equipment No.

接收日期 2021 年 12 月 09 日
Date of Receipt Y M D

结果 见校准结果
Results Show in the results of calibration

校准日期 2021 年 12 月 10 日
Date of calibration Y M D

批准人 何洪波
Approved Signatory

核 验 齐海军
Reviewed by

校 准 张东顺
Calibrated by



证书专用章
Stamp



东莞地址: 广东省东莞市石排镇东园大道石排段152号 邮政编码: 523343

电话: (0769)22200760 传真: (0769)22692542 E-mail: yws@scmdg.com.cn

Add: No.152, Shipai Duan, Dongyuan Road, Shipai Town, Dongguan, Guangdong, China.

Post Code: 523343 Tel: (0769)22200760 Fax: (0769)22692542



说 明

证书编号 GDDE202101191
Certificate No.

DIRECTIONS

第 2 页, 共 7 页
Page of

- 本中心是国家市场监督管理总局在华南地区设立的国家法定计量检定机构, 本中心的质量管理体系符合 ISO/IEC 17025:2017 标准的要求。
This laboratory is the National Legal Metrological Verification Institution in southern China set up by the General Administration of Quality Supervision. The quality system is in accordance with ISO/IEC 17025:2017.
- 本中心所出具的数据均可溯源至国家计量基准和/或国际单位制(SI)。
All data issued by this laboratory are traceable to national primary standards and/or International System of Units (SI)
- 校准地点、环境条件:
Place and environmental conditions of the calibration:
地点 本院电学实验室 温度 20 °C 相对湿度 50 %
Place Temperature RH
- 本次校准的技术依据:
Reference documents for the calibration:
JJG 1005-2019 电子式绝缘电阻表检定规程 V.R. of Electronic Insulating Resistance Meters

5. 本次校准所使用的主要计量标准器具:

Major standards of measurement used in the calibration:

设备名称/型号规格 Name of Equipment /Model/Type	编号 Serial No.	证书号/有效期/溯源单位 Certificate No./Due Date /Traceability to	计量特性 Metrological Characteristic
兆欧表检定装置 /ZX119-8C	160245	DYQ202100826 /2022-04-14 /本中心	电阻:0.1级, 电压:1级
高压高值电阻器 /TG100	1222	DYQ202100119 /2022-01-20 /本中心	2级

注: 1. 本证书校准结果只与受校准仪器有关。 The results relate only to the items calibrated.
Note: 2. 未经本机构书面批准, 不得部分复制此证书。 This certificate shall not be reproduced except in full, without the written approval of our laboratory.
3. “委托方”、“委托方联络信息”由委托方提供, “制造厂”、“型号规格”、“出厂编号”以及“设备编号”为仪器上标注。 The information Client and Contact Information are provided by client, and the Manufacturer, Model/Type, Serial No. and Equipment No. are marked on the items.
4. 本证书发布日期为2021/12/31。 The certificate is issued on 2021/12/31.



校准结果

RESULTS OF CALIBRATION

证书编号 GDDE202101191
Certificate No.

原始记录号 202101135
Record No.

第 3 页, 共 7 页
Page of

一、示值误差(电阻): 见表1

Error value(resistance): Shown in table 1

表1 Table 1

测试条件 Test condition	标准值 Reference Value	指示值 Indication Value	误差 Error	最大 允许误差 MPE	结论 Conclusion	
(V)	(MΩ)	(MΩ)	(MΩ)	(MΩ)	P/F	
500	2.00	2.03	0.03	±0.15	Pass	
	5.00	5.05	0.05	±0.30	Pass	
	10.00	10.06	0.06	±0.55	Pass	
	20.0	20.0	0.0	±1.5	Pass	
	50.0	50.1	0.1	±3.0	Pass	
	100.0	100.4	0.4	±5.5	Pass	
	200	199	-1	±15	Pass	
	500	500	0	±30	Pass	
	(GΩ)	(GΩ)	(GΩ)	(GΩ)	P/F	
	1.00	1.00	0.00	±0.10	Pass	
	2.00	2.00	0.00	±0.15	Pass	
	5.00	5.01	0.01	±0.30	Pass	
	10.00	10.00	0.00	±1.10	Pass	
	20.0	19.9	-0.1	±3.0	Pass	
50.0	49.6	-0.4	±6.0	Pass		
(V)	(MΩ)	(MΩ)	(MΩ)	(MΩ)	P/F	
	1000	2.00	1.99	-0.01	±0.15	Pass
	5.00	5.06	0.06	±0.30	Pass	
	10.00	10.10	0.10	±0.56	Pass	
	20.0	20.1	0.1	±1.5	Pass	
	50.0	50.1	0.1	±3.0	Pass	
	100.0	100.3	0.3	±5.5	Pass	
	200	201	1	±15	Pass	
	500	500	0	±30	Pass	



校准结果

RESULTS OF CALIBRATION

证书编号 GDDE202101191
Certificate No.

原始记录号 202101135
Record No.

第 4 页, 共 7 页
Page of

续表1 Table 1

测试条件 Test condition	标准值 Reference Value	指示值 Indication Value	误差 Error	最大 允许误差 MPE	结论 Conclusion
(V)	(GΩ)	(GΩ)	(GΩ)	(GΩ)	P/F
1000	1.00	1.00	0.00	±0.10	Pass
	2.00	2.01	0.01	±0.15	Pass
	5.00	5.02	0.02	±0.30	Pass
	10.00	10.02	0.02	±0.55	Pass
	20.0	20.0	0.0	±3.0	Pass
	50.0	49.8	-0.2	±6.0	Pass
	100.0	99.5	-0.5	±11.0	Pass
(V)	(MΩ)	(MΩ)	(MΩ)	(MΩ)	P/F
2500	10.00	10.09	0.09	±0.55	Pass
	20.0	20.1	0.1	±1.5	Pass
	50.0	50.6	0.6	±3.0	Pass
	100.0	100.5	0.5	±5.5	Pass
	200	201	1	±15	Pass
	500	503	3	±30	Pass
	(GΩ)	(GΩ)	(GΩ)	(GΩ)	P/F
	1.00	1.00	0.00	±0.10	Pass
	2.00	2.01	0.01	±0.15	Pass
	5.00	5.03	0.03	±0.30	Pass
	10.00	10.07	0.07	±0.55	Pass
	20.0	20.1	0.1	±1.5	Pass
	50.0	50.2	0.2	±8.5	Pass
	100.0	100.1	0.1	±16.0	Pass
	200	200	0	±40	Pass



校准结果

RESULTS OF CALIBRATION

证书编号 GDDE202101191
Certificate No.

原始记录号 202101135
Record No.

第 5 页, 共 7 页
Page of

续表1 Table 1

测试条件	标准值	指示值	误差	最大允许误差	结论	
Test condition	Reference Value	Indication Value	Error	MPE	Conclusion	
(V)	(MΩ)	(MΩ)	(MΩ)	(MΩ)	P/F	
5000	100.0	101.6	1.6	±5.6	Pass	
	200	201	1	±15	Pass	
	500	505	5	±30	Pass	
	(GΩ)	(GΩ)	(GΩ)	(GΩ)	P/F	
	1.00	1.01	0.01	±0.10	Pass	
	2.00	2.01	0.01	±0.15	Pass	
	5.00	5.04	0.04	±0.30	Pass	
	10.0	10.1	0.1	±1.0	Pass	
	20.0	20.1	0.1	±1.5	Pass	
	50.0	50.5	0.5	±3.0	Pass	
10000	100.0	101.3	1.3	±17.2	Pass	
	200	199	-1	±50	Pass	
	500	497	-3	±95	Pass	
	(V)	(MΩ)	(MΩ)	(MΩ)	(MΩ)	P/F
	10000	100.0	101.6	1.6	±11.2	Pass
		200	204	4	±30	Pass
		500	505	5	±61	Pass
		(GΩ)	(GΩ)	(GΩ)	(GΩ)	P/F
		1.00	1.01	0.01	±0.20	Pass
		2.00	2.03	0.03	±0.30	Pass
5.00		5.04	0.04	±0.60	Pass	
10.0		10.1	0.1	±2.0	Pass	
20.0		20.3	0.3	±3.0	Pass	
50.0		50.6	0.6	±6.1	Pass	



校准结果

RESULTS OF CALIBRATION

证书编号 GDDE202101191
Certificate No.

原始记录号 202101135
Record No.

第 6 页, 共 7 页
Page of

续表1 Table 1


测试条件	标准值	指示值	误差	最大 允许误差	结论
Test condition	Reference Value	Indication Value	Error	MPE	Conclusion
(V)	(GΩ)	(GΩ)	(GΩ)	(GΩ)	P/F
10000	100.0	101.5	1.5	±11.2	Pass
	200	208	8	±31	Pass
	500	510	10	±61	Pass
	1000	986	-14	±109	Pass

二、开路电压（电压）：见表2

Open circuit voltage (voltage) : Shown in table 2

表2 Table 2

标准值	指示值	结论
Reference Value	Indication Value	Conclusion
(V)	(V)	
514	500	N/A
1043	1000	N/A
2559	2500	N/A
5238	5000	N/A
10180	10000	N/A

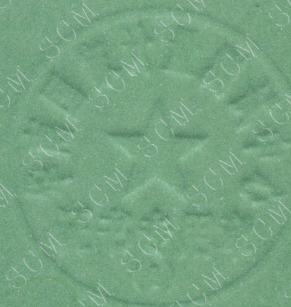



校准结果

RESULTS OF CALIBRATION

证书编号 GDDE202101191
Certificate No.

原始记录号 202101135
Record No.

第 7 页, 共 7 页
Page of

说明:

Note:

1. 本次测量结果的扩展不确定度:

The Expanded Uncertainty of Measurement:

电阻: $U_{rel}=1.6\%(\leq 1G\Omega)$, $U_{rel}=3\%(\leq 2T\Omega)$; 电压: $U_{rel}=3\%$;

包含因子 $k=2$, 本证书中给出的扩展不确定度依据JJF1059.1-2012《测量不确定度评定与表示》评定, 由合成标准不确定度乘以包含概率约为95%时对应的包含因子 k 得到。

Coverage factor $k=2$, the expanded uncertainty given in this certificate is evaluated according to JJF 1059.1-2012 "Evaluation and Expression of Uncertainty in Measurement", which is obtained by multiplying the combined standard uncertainty by the coverage factor k corresponding to the coverage probability of about 95%.

2. 判定准则为JJF1094-2002《测量仪器特性评定》第5.3.1条款和该仪器说明书技术要求。

Decision criteria is JJF1094-2002《Evaluation of the Characteristics of Measuring Instruments》 and the technical requirements in the manual.

3. 按照所依据技术文件的规定, 建议复校时间间隔不超过1年。

According to the demand of reference document, next calibration is proposed within 1 year.

4. 更改内容: 计量器具名称“电子式绝缘电阻表”更改为: “10kV高压绝缘电阻测试仪(电子式绝缘电阻表)”, 原证书作废。

