


UT276A+ QA测试报告

使用检测设备:电阻箱

环境温湿度:24.9℃/65.1%

功能	量程	输入	准确度	最大允许误差	读数范围	实际测量值	结果
Ω	0.01Ω ~1200Ω	0.01Ω	±(1%+0.01)	±0.01Ω	0.00~0.02Ω	10.01Ω	Pass
		0.05Ω		±0.01Ω	0.04~0.06Ω	0.042Ω	Pass
		1.0Ω	±(1%+0.1)	±0.1Ω	0.9~1.1Ω	0.9Ω	Pass
		4.5Ω		±0.2Ω	4.3~4.7Ω	4.4Ω	Pass
		10.0Ω		±0.2Ω	9.8~10.2Ω	9.8Ω	Pass
		30.0Ω		±0.4Ω	29.6~30.4Ω	29.8Ω	Pass
		50.0Ω		±0.6Ω	49.4~50.6Ω	49.7Ω	Pass
		95.0Ω		±1.1Ω	93.9~96.1Ω	94.5Ω	Pass
		150Ω	±(5%+5)	±13Ω	137~163Ω	149Ω	Pass
		450Ω	±(10%+10)	±55Ω	395~505Ω	440Ω	Pass
		750Ω	±(20%+20)	±170Ω	580~920Ω	700Ω	Pass
		950Ω	±(25%+30)	±268Ω	682~1218Ω 或0L	880Ω	Pass
		1000Ω		±280Ω	720~1280Ω 或0L	920Ω	Pass
		1200Ω		±330Ω	870~1530Ω 或0L	1080Ω	Pass

备注:钳头铁芯由精密磁性材料制作,在测试时要小心张合钳口中,严禁撞击钳口,以免损坏钳表.

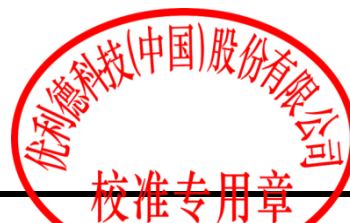

检验员:张琼

审核员:郭桂东